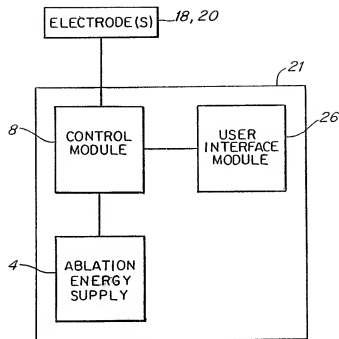


*Fig. 1*

*Fig. 2**Fig. 3**Fig. 4*



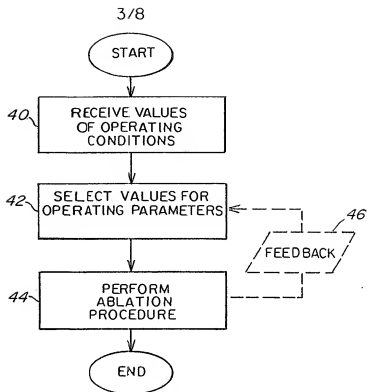


Fig. 5

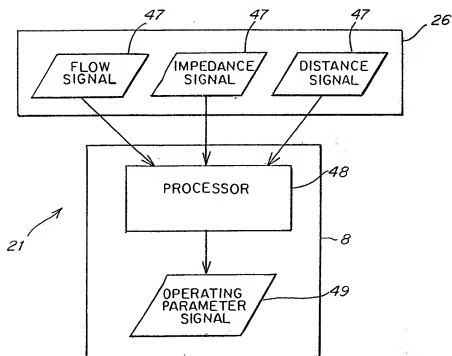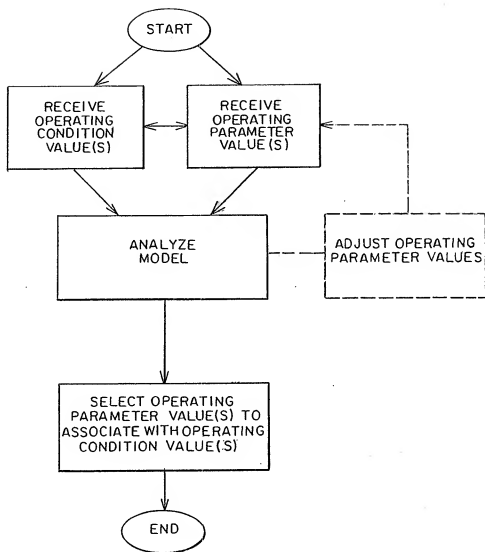

Fia. 6

*Fig. 7*

5/8




Fig. 8

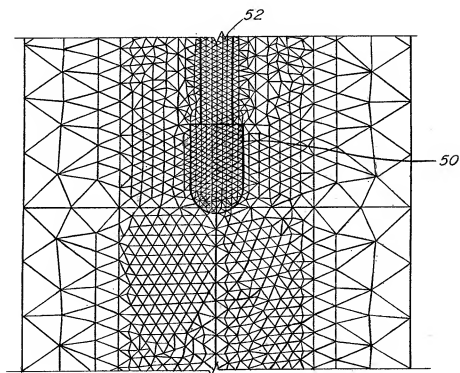


Fig. 9

Power vs. Maximum Tissue Temperature
30 mm/sec (2.9 L/min)

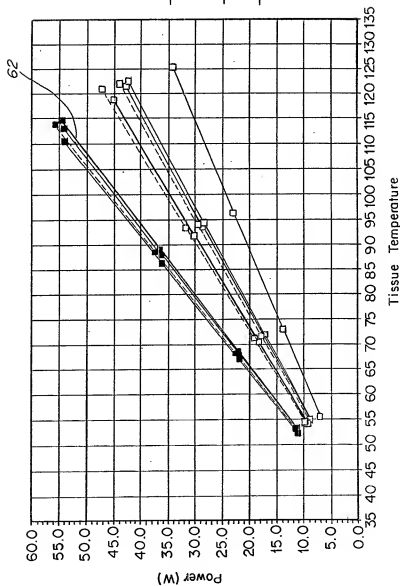


Fig. 10

Maximum Electrode Temperature vs. Maximum Tissue Temperature
 30 mm/sec (2.9 L/min)

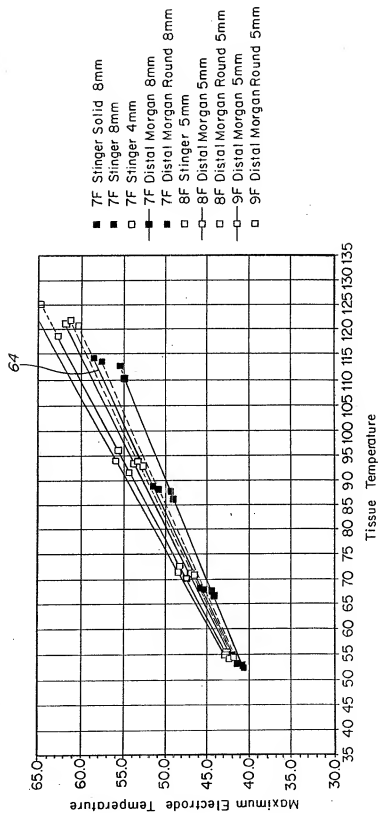


Fig. 11

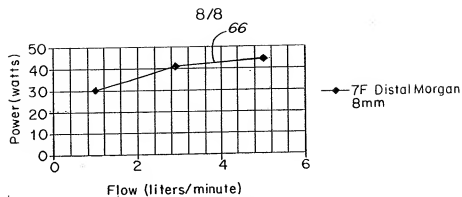


Fig. 12A

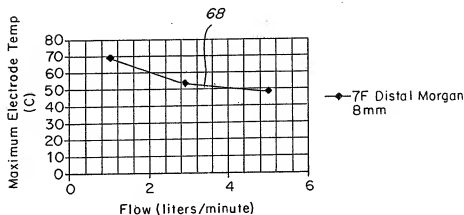


Fig. 12B

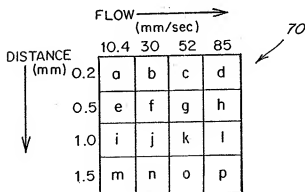


Fig. 13